

Telemonitoring of diabetic foot ulcers being managed in the outpatient setting

Piotr Foltynski, Piotr Ladyzynski,
Jan M Wojcicki

Article points

1. Wound area monitoring is an important element of treatment evaluation.
2. The authors describe a telemonitoring device developed to be used to image the diabetic foot ulcers of outpatients in their own homes.
3. The scanning system sends images of the wound, as well as blood pressure and glycaemic measurements, to the clinician for analysis.
4. Use of this system could have positive implications for clinical and cost-effectiveness and outpatient safety.

Keywords

- Outpatient care
- Telemonitoring
- Wound area monitoring
- Wound imaging

Author details can be found on the last page of this article.

Wound assessment and monitoring is an important element of managing diabetic foot ulcers. However, wounds managed in the outpatient setting are assessed by the clinician less frequently than those among inpatients, leaving the outpatient exposed to lengthier periods of ineffective treatment and the possibility of undetected life- and limb-threatening wound deterioration between clinic appointments. The authors describe a mobile, patient-operated device that allows the clinician to remotely monitor wounds. This device has a number of potential applications in the community-based management of diabetic foot ulceration.

It is widely agreed that diabetic foot ulcers require careful monitoring during healing, and that the monitoring of wound area is an important element of wound treatment evaluation (Sheehan et al, 2003; Cardinal et al, 2008; Lavery et al, 2008; Coerper et al, 2009). While the monitoring of wounds is straightforward in the inpatient setting, the majority of chronic diabetic foot ulcers are managed in the community setting where regular assessment is more difficult to coordinate. To reduce the risks and inconveniences associated with the management of diabetic foot ulcers in the community setting, innovative interventions need to be designed. In this vein, the authors developed a patient-operated, at-home wound imaging device. The device, a

pilot trial, and a discussion of its potential applications are described here.

Digital wound imaging

A number of devices designed for wound imaging are available, but are not designed to be operated by patients (Plassmann and Jones, 1998; Körber et al, 2006; Ahn and Salcido, 2008; Romanelli et al, 2008). By contrast, the authors' wound imaging device – the TeleDiaFoS patient module (*Figure 1*) – is designed for use by the patient, in his or her own home.

The design goals for the device were to:

- Improve outpatient safety by allowing remote wound assessment by the clinician.
- Produce a wound image of acceptable quality for the purposes of clinician assessment, but of a small enough digital

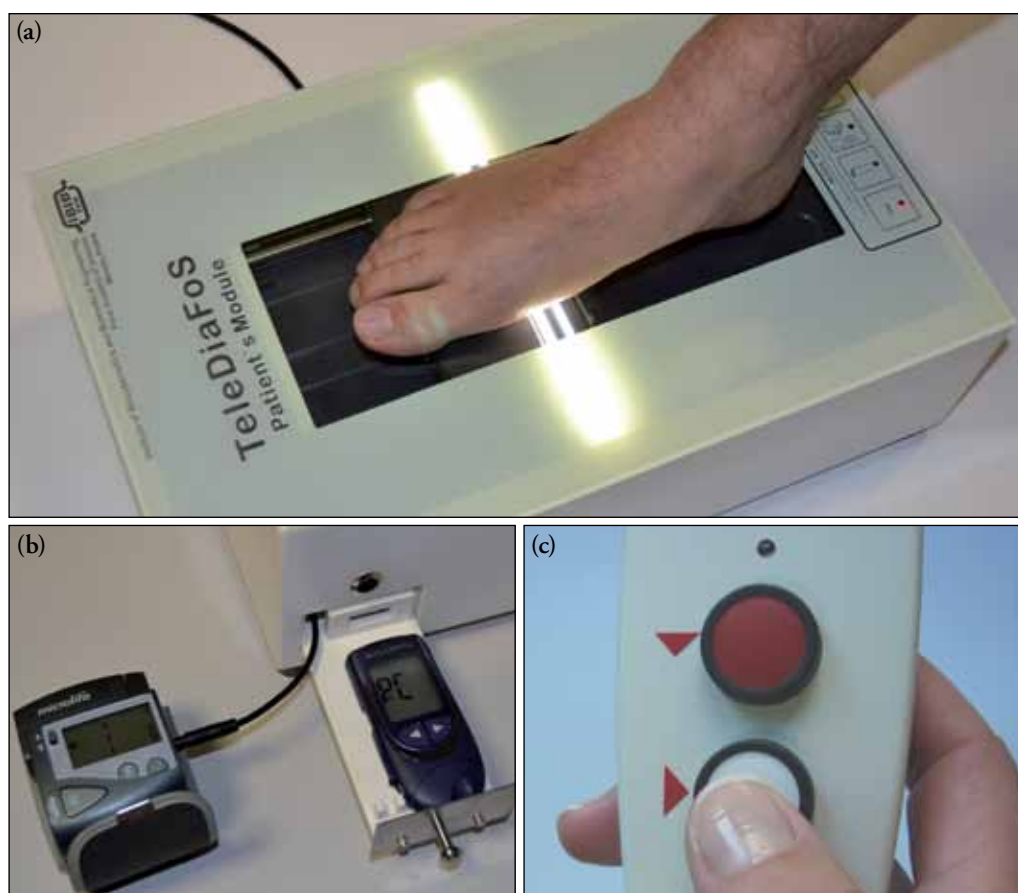


Figure 1. The TeleDiaFoS patient module is designed to (a) scan an image of a foot ulcer and (b) assess blood pressure and blood glucose levels. These data are transmitted to the clinician for assessment. (c) The module is operated by a one-touch remote control.

file size to allow rapid data collection and transfer.

- Retrieve and transmit data from blood glucose and blood pressure meters for assessment.
- Be easy for patients to operate, unassisted, in their own home.

The module comprises a foot wound scanning window (tempered glass), a blood glucose meter (Accu-Chek; Roche, Germany) and a blood pressure monitor (3BU1-4PC; Microlife, Switzerland). The use of the wound scanning element is the focus of this article.

To use the module, the patient places it on the floor, switches it on, and disinfects the scanning window with a hospital-quality disinfectant before use. The patient then removes the dressing, applies an appropriate skin sanitiser spray to the foot and places the foot on the scanning window (*Figure 1a*). The patient initiates the scan using the hand-

held, one touch remote control (*Figure 1c*). The module scans the foot in approximately 15 seconds.

The module's internal modem (not reliant on a phone or internet connection within the patient's home) automatically transmits the data either to the clinician's server or to an email to addresses specified in advance. The clinician then views the image (*Figure 2*) and evaluates the wound's appearance (as well as the patient's glycaemia and blood pressure, if these functions are being used).

If the transmitted image is viewed through the TeleDiaFoS software, it quantifies wound area based on the area of a polygon traced on the wound edges (*Figure 3*). The software also calculates the change in wound area from previous images (i.e. over the course of treatment) and provides a graph of wound area over time.

The cost of the module is approximately US\$2500, based on the manufacture

Figure 2. Sample image of a patient's sole with wound taken by the patient's module device.



of a handful of units for the feasibility assessment. However, were the production to run to of thousands of units, the authors predict the cost would drop to less than US\$1000 per device.

Evidence for use

The module was tested on 10 people with type 2 diabetes, peripheral neuropathy and an active foot ulcer on one foot only (Foltynski et al, 2011a; 2011b). Participants were shown how to use the module at a clinic appointment or in their home and then

asked to use the module at every self-dressing change over a 3-month period or until the wound healed. Each image was evaluated by four observers in order to confirm calculated wound area and area change over time.

All participants were able to operate the module. Seven images out of 386 (1.8%) were lost owing to interruption of internet connection, but were retrieved from the backup memory of the module. This pilot study confirmed the usefulness of the module and its acceptability to users.

Discussion

The use of telemonitoring in the management of chronic conditions has been identified as a promising health improvement tool; when used appropriately, telemonitoring is able to produce accurate and reliable data, empower patients, reduce costs, and improve outcomes (Paré et al, 2007). The module described here is an example of a telemonitoring intervention with the potential to improve clinical and cost-effectiveness.

There are a number of applications for the module described here. Broadly, it can provide benefits to the clinician, patient and health service by:

- Decreasing the frequency of unnecessary clinic visits by outpatients.
- Decreasing the frequency of unnecessary home visits by clinicians to people being managed in the community.
- Rapid cessation of ineffective therapies.
- Rapid recognition of, and clinical intervention to address, deteriorating wounds.
- Providing rapid access to clinical opinions on wounds for people living in isolated regions and people with mobility issues (e.g. elderly, frail, obese or otherwise house-bound people, people in assisted living facilities).

Limitations

Accurately rendering a three-dimensional object into a two-dimensional image, as this system seeks to do, is a difficult



Figure 3. A screenshot of the TeleDiaFoS software used to calculate wound area.

process. Wound area has been shown to be subjective, with clinicians differing in their opinion on where wound margins should be drawn (Flanagan, 2003). For example callus, hyperkeratosis, dried exudate and ulcers that undermine or track through ostensibly healthy tissue can obscure the extent of wound area and depth.

The smaller the angle between the plane in which the wound is lying and the scanning plane, the larger is the area reproducible by the scanner. For this reason, although not limited to scanning the sole of the foot, the module is most successful for imaging plantar wounds (Foltynski et al, 2011b).

A randomised controlled trial is needed to fully assess the clinical and cost-effectiveness of the module.

Conclusion

Remote wound imaging devices, such as the TeleDiaFoS patient module described here, have the potential to provide clinical and cost-effective improvements in the community-based care of people with chronic diabetic foot ulcers. Such devices are promising applications that integrate communication and medical technologies and are worthy of larger-scale investigations. ■

Authors

Piotr Foltynski is a Senior Researcher, Piotr Ladyzynski is Associate Professor of Biomedical Engineering and Jan M Wojcicki is Professor of Biomedical Engineering; all are based at the Nalecz Institute of Biocybernetics and Biomedical Engineering, Polish Academy of Sciences, Warsaw, Poland.

Ahn C, Salcido RS (2008) Advances in wound photography and assessment methods. *Adv Skin Wound Care* **21**: 85–93

Cardinal M, Eisenbud DE, Phillips T, Harding K (2008) Early healing rates and wound area measurements are reliable predictors of later complete wound closure. *Wound Repair Regen* **16**: 19–22

Coerper S, Beckert S, Küper MA et al (2009) Fifty percent area reduction after 4 weeks of treatment is a reliable indicator for healing – analysis of a single-center cohort of 704 diabetic patients. *J Diabetes Complications* **23**: 49–53

Flanagan M (2003) Improving accuracy of wound measurement in clinical practice. *Ostomy Wound Manage* **49**: 28–40

Foltynski P, Wojcicki JM, Ladyzynski P et al (2011a) Monitoring of diabetic foot syndrome treatment: some new perspectives. *Artif Organs* **35**: 176–82

Foltynski P, Ladyzynski P, Migalska-Musial K et al (2011b) A new imaging and data transmitting device for telemonitoring of diabetic foot syndrome patients. *Diabetes Technol Ther* **13**: 861–7

Körber A, Rietkötter J, Grabbe S, Dissemund J (2006) Three-dimensional documentation of wound healing: first results of a new objective method for measurement. *J Dtsch Dermatol Ges* **4**: 848–54

Lavery LA, Barnes SA, Keith MS et al (2008) Prediction of healing for postoperative diabetic foot wounds based on early wound area progression. *Diabetes Care* **31**: 26–9

Paré G, Jaana M, Sicotte C (2007) Systematic review of home telemonitoring for chronic diseases: the evidence base. *J Am Med Inform Assoc* **14**: 269–77

Plassmann P, Jones TD (1998) MAVIS: a non-invasive instrument to measure area and volume of wounds. *Med Eng Phys* **20**: 332–8

Romanelli M, Dini V, Rogers L et al (2008) Clinical evaluation of a wound measurement and documentation system. *Wounds* **20**: 256–64

Sheehan P, Jones P, Caselli A et al (2003) Percent change in wound area of diabetic foot ulcers over a 4-week period is a robust predictor of complete healing in a 12-week prospective trial. *Diabetes Care* **26**: 1879–82